

MONTHLY REPLACEMENT

XTENSA RX





HYDROGEL



PARAMETERS

| | |
|-------------------------|--|
| Base curves (mm) | SPH, MF 8.50 TOR, MFT 8.70 |
| Diameter (mm) | 14.40 |
| Spheres (D) | SPH ± 30.00 (0.50 after ± 6.00) TOR, MF, MFT ± 30.00 (0.50 after $+4.00/-6.00$) |
| Cylinders | -0.75 to -7.75 (0.50) |
| Axes (°) | All (5°) |
| Additions | CD +1.50/+2.50 CN +1.25/+2.25 |

OPTICAL DESIGN

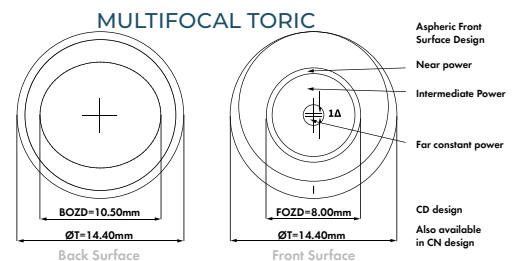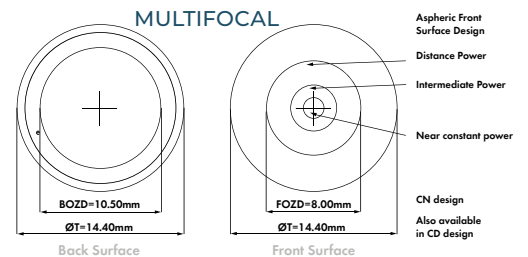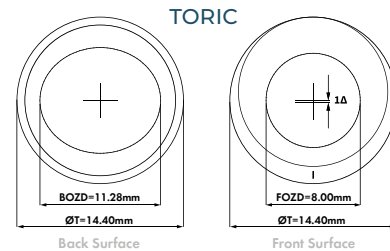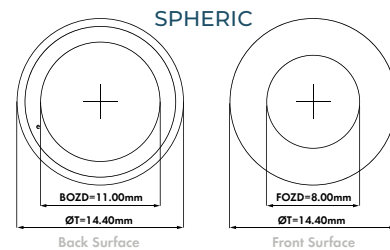

Lens design parameters may change depending on the power

MATERIAL

| | |
|------------------------------------|---------------------|
| Type | Filcon 4 (19) [55%] |
| DK (ISO 9913-1-1998) | 19 |
| DK/t (-3.00 D) | 19 |
| Water Content | 55% |
| Central Thickness (-3.00 D) | 0.10 |
| Handling tint | Blue |
| Pack size | 6 Lenses |
| Manufacturing Process | Lathed |